

Journal of Advanced Research in Applied Sciences and Engineering Technology

Journal homepage: https://semarakilmu.com.my/journals/index.php/applied_sciences_eng_tech/index ISSN: 2462-1943



Comparative Analysis between Three Reliability Models of a Two-Unit Complex Industrial System

Syed Zegham Taj^{1,*}, Syed Mohammed Rizwan¹

Department of Applied Mathematics and Science, National University of Science and Technology, Sultanate of Oman

ARTICLE INFO ABSTRACT Article history: This paper presents the reliability modelling and analysis of a complex industrial system Received 12 December 2022 with two units operating in parallel. To facilitate the study, real failure-maintenance Received in revised form 20 March 2023 data of the system are collected. Data depicts that a unit is repaired upon failure by a Accepted 5 April 2023 single repairman. Reliability indices of the system such as mean time between failures, Available online 24 April 2023 availability, expected number of repairs, and expected busy period of the repairman are estimated using semi-Markov processes and regenerative processes. Finally, a Keywords: comparative analysis between the reliability indices of three reliability models for the Availability; semi-Markov processes; system is presented. regenerative processes; reliability

1. Introduction

Numerous researchers have contributed to the field of reliability modelling and analysis while analyzing complex industrial systems under different operating conditions and assumptions.

Rizwan and Taneja [1] estimated the profit of a system with perfect repair, partial failure and complete failure. In a study, Rizwan et al., [2] carried out a comparative study between the profits of two models for a two-unit system that incorporates a rest period for the repairman. In another study, Rizwan et al., [3] introduced the concept of an accident during the inspection and the possibility of multiple post-repair inspections while examining one-unit and two-unit systems. Later, Rizwan et al., [4-6] extensively analyzed PLC systems with a single unit and hot standby, various reliability indices and profit incurred were estimated. Rizwan [7] also performed a reliability analysis of a two-unit system with two repairmen. A detailed analysis of a CC plant was reported by Mathew et al., [8,9] to estimate key performance indicators such as mean time to system failure, availability, etc. Mathew et al., [10-14] continued to work on the CC plant with scheduled maintenance policy, different installed capacities, full installed capacity, and profit evaluation; and presented a comparative analysis between profits of two models of the CC plant. In several studies, Padmavathi et al., [15-19] analyzed a desalination plant with online repair and emergency shutdowns, with minor/major failures and priority given to repairing over maintenance, with major and minor failures and

E-mail address: syedtaj@nu.edu.om

-

https://doi.org/10.37934/araset.30.2.243254

^{*} Corresponding author.

shutdown during the winter season, and finally presented a comparative analysis of two models of the desalination plant. To examine to a greater extent the desalination plant with mandatory shutdown during winter season and repair/maintenance on FCFS basis and compare the various reliability models of the desalination plant, the methodology was [20-22]. Subsequently, analysis of a wastewater treatment plant and an anaerobic batch reactor was presented; reliability indices of interest were estimated to assess the plant/reactor performance [23-25]. Rizwan and Mathew [26] extended their work for the performance analysis of port cranes. A detailed study of the aluminium industry was presented by Al Rahbi et al., [27-32], wherein, the butt thimble removal station and rodding anode plant were analyzed for important reliability indices. Later, Al Rahbi and Rizwan [33] presented a comparative analysis between the models of a single component with a single repairman and multiple repairmen in the aluminium industry. Taj et al., [34-39] carried out a detailed reliability analysis of a cable plant and its subsystems with different maintenance categories, storage of surplus produce, season based operating strategy, and presented a comparative analysis between three profit models of the cable plant. Taj and Rizwan [40] critically reviewed the reliability modelling and analysis of complex industrial systems, whereas Rizwan and Taj [41] presented reliability modeling and analysis of port PLCs. Kunalan et al., [42] investigated the performance of a multi-staging hydrokinetic turbine for river flow. Taj and Rizwan [43,44] further discussed the reliability analysis of a system using best-fit distributions for repair/restoration times, and a 3-unit parallel system with a single maintenance facility, respectively.

Hence, the methodology for reliability modelling and analysis of complex industrial systems under various failure/maintenance situations has been widely presented in the literature.

In this paper, reliability modelling and analysis of a complex industrial system with two units operating in parallel is presented. Real failure-maintenance data of the system shows that a failed unit undergoes repair by a single repairman. Using semi-Markov processes and regenerative processes, important reliability indices of the system namely mean time between failures, availability, expected number of repairs, and expected busy period of the repairman are estimated. Recently, Taj et al., [45,46] analyzed two reliability models of the system under different operating conditions and assumptions. Thus, a comparative analysis between the reliability indices of the three reliability models for the system is also presented in this paper. The analysis is useful in deducing the suitability of one model over the other.

2. Model Description (Model I)

The following operating conditions and assumptions are considered

- i. The system consists of two units.
- ii. The units operate in parallel.
- iii. A unit is repaired upon failure.
- iv. After each repair, the failed unit regenerates.
- v. There is only one repairman.
- vi. Repair times are assumed to be arbitrarily distributed.
- vii. Failure times are assumed to be exponentially distributed.

State-transition table of the system is shown in Table 1. Zero (0) stands for no transition to the mentioned state.

Table 1State-transition table

State transition table						
	Sj	S ₀	S ₁	S ₂		
Si						
S ₀		0	$2\lambda_1$	0		
S_1		$g_1(t)$	0	λ_1		
S ₂		0	$g_1(t)$	0		
For non-regenerative state S ₂						
$S_1 \text{ to } S_1 \text{ via } S_2 \qquad q_{11}^2(t) = (\lambda_1 e^{-\lambda_1 t} \odot 1) g_1(t)$						

States of the system are described below

S₀: both units are operative.

 S_1 : one unit has failed and is under repair; one unit is operative.

S₂: one unit has failed and is under repair from the previous state; one unit has failed and is waiting for repair.

here,

 S_0 and S_1 are regenerative states.

S₂ is the non-regenerative state as well as the failed state.

Note: System is considered to be in the failed state when both units have failed.

3. Transition Probabilities and Mean Sojourn Times

Using the definition of transition probabilities $q_{ij}(t)$, we get [47]

$$q_{01}(t) = 2\lambda_1 e^{-2\lambda_1 t} \tag{1}$$

$$q_{10}(t) = g_1(t)e^{-\lambda_1 t}$$
 (2)

$$q_{12}(t) = \lambda_1 e^{-\lambda_1 t} \overline{G_1}(t) \tag{3}$$

$$q_{11}^2(t) = \left(\lambda_1 e^{-\lambda_1 t} \odot 1\right) g_1(t) \tag{4}$$

$$q_{21}(t) = g_1(t)$$
 (5)

where,

 $G_1(t)$ denotes the cdf of repair times.

Using the definition of non-zero elements p_{ij} , we get [47]

$$p_{01} = \frac{2\lambda_1}{2\lambda_1} \tag{6}$$

$$p_{10} = g_1^*(\lambda_1) \tag{7}$$

$$p_{12} = 1 - g_1^*(\lambda_1) \tag{8}$$

$$p_{11}^2 = 1 - g_1^*(\lambda_1) \tag{9}$$

$$p_{21} = g_1^*(0) (10)$$

The following can be easily verified

$$p_{01} = 1 (11)$$

$$p_{10} + p_{12} = 1 (12)$$

$$p_{10} + p_{11}^2 = 1 (13)$$

$$p_{21} = 1 (14)$$

Using the definition of mean sojourn time μ_i , we get [47]

$$\mu_0 = \frac{1}{2\lambda_1} \tag{15}$$

$$\mu_1 = \int_0^\infty \overline{G_1}(t) e^{-\lambda_1 t} dt \tag{16}$$

$$\mu_2 = \int_0^\infty \overline{G_1}(t)dt \tag{17}$$

Using the definition of unconditional mean time m_{ij} , following can be easily verified [47]

$$m_{01} = \mu_0 \tag{18}$$

$$m_{10} + m_{12} = \mu_1 \tag{19}$$

$$m_{10} + m_{11}^2 = \mu_2 \tag{20}$$

$$m_{21} = \mu_2$$
 (21)

4. Mean Time Between Failures

Using simple probabilistic arguments and the definition of $\phi_i(t)$, we get [47]

$$\phi_0(t) = Q_{01}(t) \$ \phi_1(t) \tag{22}$$

$$\phi_1(t) = Q_{10}(t) \cdot \phi_0(t) + Q_{12}(t) \tag{23}$$

Taking LST of the above equation and solving for $\varphi_0^{**}(s)$, we obtain

$$\phi_0^{**}(s) = \frac{N(s)}{D(s)}$$
 (24)

The MTBF, given that the system started at the beginning of state 0 is given by

MTBF =
$$\lim_{s \to 0} \frac{1 - \phi_0^{**}(s)}{s} = \frac{N}{D}$$
 (25)

where,

$$N = \mu_0 + \mu_1 \tag{26}$$

$$D = p_{12} \tag{27}$$

5. Availability of the System

Using simple probabilistic arguments and the definition of $A_i(t)$, we get [47]

$$A_0(t) = M_0(t) + q_{01}(t) @ A_1(t)$$
(28)

$$A_1(t) = q_{10}(t) \otimes A_0(t) + q_{11}^2 \otimes A_1(t)$$
(29)

where,

$$M_0(t) = e^{-2\lambda_1 t} \tag{30}$$

Taking LT of the above equations and solving for $A_0^*(s)$, we get

$$A_0^*(s) = \frac{N_1(s)}{D_1(s)} \tag{31}$$

In steady state, the availability of the system is given by

$$A_0 = \lim_{s \to 0} s \, A_0^*(s) = \frac{N_1}{D_1} \tag{32}$$

where,

$$N_1 = p_{10}\mu_0 \tag{33}$$

$$D_1 = p_{10}\mu_0 + \mu_2 \tag{34}$$

6. Expected Busy Period of the Repairman

Using simple probabilistic arguments and the definition of $B_i(t)$, we get [47]

$$B_0(t) = q_{01}(t) \otimes B_1(t)$$
(35)

$$B_1(t) = W_1(t) + q_{10}(t) @ B_0(t) + q_{11}^2(t) @ B_1(t)$$
(36)

where,

$$W_1(t) = e^{-\lambda_1 t} \overline{G_1}(t) \tag{37}$$

Taking LT of above equations and solving for $B_0^*(s)$, we obtain

$$B_0^*(s) = \frac{N_2(s)}{D_1(s)} \tag{38}$$

In steady state, the expected busy period of the repairman is given by

$$B_0 = \lim_{s \to 0} s \, B_0^*(s) = \frac{N_2}{D_1} \tag{39}$$

where,

$$N_2 = W_1^*(0) (40)$$

 D_1 is specified in Eq. (34).

7. Expected Number of System Repairs

Using simple probabilistic arguments and the definition of $R_i(t)$, we get [47]

$$R_0(t) = Q_{01}(t) \$ \{R_1(t) + 1\}$$
(41)

$$R_1(t) = Q_{10}(t) SR_0(t) + Q_{11}^2(t) S\{R_1(t) + 1\}$$
(42)

Taking LST of the above equations and solving for $R_0^{\ **}(s)$, we get

$$R_0^{**}(s) = \frac{N_3(s)}{D_1(s)} \tag{43}$$

In steady state, the expected number of system repairs is given by

$$R_0 = \lim_{s \to 0} s \, R_0^{**}(s) = \frac{N_3}{D_1} \tag{44}$$

where,

$$N_3 = 1 \tag{45}$$

 D_1 is specified in Eq. (34).

8. Particular Case

As a particular case, we assume that the repair times also follow exponential distribution, let us say

$$g_1(t) = \gamma_1 e^{-\gamma_1 t} \tag{46}$$

Table 2 shows the values of various rates estimated from the real-maintenance failure data of the system.

Table 2Estimated values of rates for the system

S. No.	Rate	Value (per hour)			
1	constant failure rate, λ_1	0.00368			
2	constant repair rate, γ_1	0.24729			

Substituting the above table values in the expressions obtained in sections 4 to 7, following reliability indices of the system are obtained

Mean time between failures: 2063 hours (47)	17	")	
---	----	----	--

Availability of the system: 0.901 (48)

Expected number of system repairs: 0.016 (49)

Expected busy period of the repairman: 0.062 (50)

9. Previous Work

Earlier, two reliability models of the system under consideration were analysed by Taj *et al.*, [45,46] wherein different operating conditions and assumptions were taken into account.

For Model II, the following were considered (in addition to the operating conditions and assumptions of Model I) [45]

- i. Three types of maintenances are performed: repair, minor PM, and major PM.
- ii. Minor/major PM are performed at a scheduled basis.
- iii. Priority is given to repair over minor/major PM.

However for Model III, the authors considered the following (in addition to the operating conditions and assumptions of Models I and II) [46]

- i. Machines are queued for major PM.
- ii. An operative machine requires a cooling period of half hour before undergoing major PM.

For Model II, the following values of reliability indices of the system were obtained (refer Taj *et al.*, [45] for details)

Whereas for Model III, the estimated reliability indices of the system were as follows (refer Taj *et al.*, [46] for details)

10. Comparative Analysis

This section presents a comparison between the values of reliability indices of the system obtained for Model I (section 8) with those given for Models II and III (section 9).

Comparison between the values of mean time between failures for the three models is shown in Figure 1.

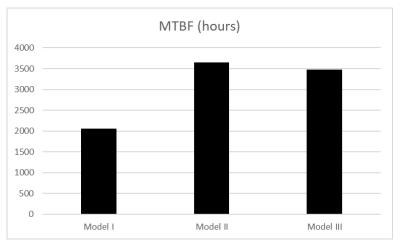


Fig. 1. Comparison between MTBF (hours)

Comparison between the values of availability of the system for the three models is shown in Figure 2.

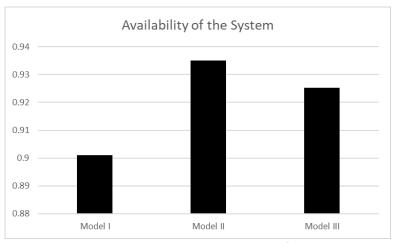


Fig. 2. Comparison between availability of the system

Comparison between the values of expected number of system repairs for the three models is shown in Figure 3.

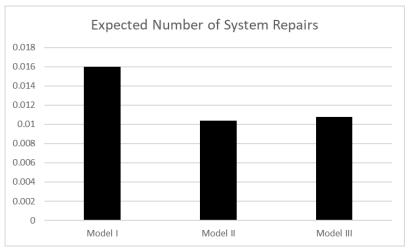


Fig. 3. Comparison between expected number of system repairs

Comparison between the values of expected busy period of the repairman for the three models is shown in Figure 4.

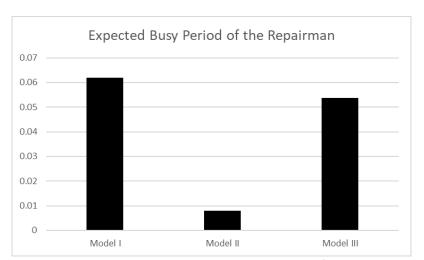


Fig. 4. Comparison between expected busy period of the repairman

From Figure 1 to Figure 4, following observations can be drawn

- i. The MTBF for Model II is more as compared to Models I and III.
- ii. The availability of the system for Model II is more as compared to Models I and III.
- iii. The expected number of system repairs for Model II is less as compared to Models I and III.
- iv. The expected busy period of the repairman for Model II is less as compared to Models I and III.

11. Conclusion

Reliability modelling and analysis of a complex industrial system with two units operating in parallel is presented. Reliability indices of the system viz. mean time between failures, availability,

expected number of repairs, and expected busy period of the repairman are estimated. Comparative analysis between the reliability indices of three reliability models of the system is presented. The comparison clearly indicates the suitability of Model II over Models I and III.

References

- [1] Rizwan, S. M., and Gulshan Taneja. "Profit analysis of a system with perfect repair at partial failure or complete failure." *Pure and Applied Mathematika Sciences* 52, no. 1/2 (2000): 7-14.
- [2] Rizwan, S. M., Gulshan Taneja, and R. K. Tuteja. "Comparative study between the profits of two models for a two unit system with rest period of repairman." *Journal of Decision and Mathematical Sciences* 5, no. 1-3 (2000): 27-44
- [3] Rizwan, S. M., Harjeet Chauhan, and Gulshan Taneja. "Stochastic analysis of systems with accident and inspection." *Emirates Journal for Engineering Research* 10, no. 2 (2005): 81-88.
- [4] Rizwan, S. M., Vipin Khurana, and Gulshan Taneja. "Reliability modeling of a hot standby PLC system." In *Proceedings of the International Conference on Communication, Computer and Power (ICCCP'05)*, Sultan Qaboos University, Sultanate of Oman, pp. 486-489. 2005.
- [5] Rizwan, S. M., Vipin Khurana, and Gulshan Taneja. "Modelling and Optimization of a Single-Unitplc System." International Journal of Modelling and Simulation 27, no. 4 (2007): 361-368. https://doi.org/10.1080/02286203.2007.11442438
- [6] Rizwan, S. M., Vipin Khurana, and Gulshan Taneja. "Reliability analysis of a hot standby industrial system." International Journal of Modelling and Simulation 30, no. 3 (2010): 315-322. https://doi.org/10.1080/02286203.2010.11442586
- [7] Rizwan, S. M. "Reliability analysis of a two unit system with two repairmen." *Caledonian Journal of Engineering* 3, no. 2 (2007): 1-5.
- [8] Mathew, A. G., S. M. Rizwan, M. C. Majumder, and K. P. Ramachandran. "MTSF and Availability of a two unit CC Plant." In *Proceedings of the International Conference on Modeling, Simulation and Applied Optimization*, pp. 1-5. 2009.
- [9] Mathew, A. G., S. M. Rizwan, M. C. Majumder, and K. P. Ramachandran. "Reliability modelling and analysis of a two unit continuous casting plant." *Journal of the Franklin Institute* 348, no. 7 (2011): 1488-1505. https://doi.org/10.1016/j.jfranklin.2010.04.016
- [10] Mathew, A. G., S. M. Rizwan, M. C. Majumder, K. P. Ramachandran, and Gulshan Taneja. "Optimization of a single unit CC plant with scheduled maintenance policy." In *Proceedings of the International Conference on Recent Advances in Material Processing Technology*, pp. 609-613. 2009.
- [11] Mathew, A. G., S. M. Rizwan, M. C. Majumder, K. P. Ramachandran, and G. Taneja. "Profit evaluation of a single unit CC plant with scheduled maintenance." *Caledonian Journal of Engineering* 5, no. 1 (2009): 25-33.
- [12] Mathew, A. G., S. M. Rizwan, M. C. Majumder, K. P. Ramachandran, and Gulshan Taneja. "Comparative analysis between profits of the two models of a CC plant." In *AIP Conference Proceedings*, vol. 1298, no. 1, pp. 226-231. American Institute of Physics, 2010. https://doi.org/10.1063/1.3516306
- [13] Mathew, A. G., S. M. Rizwan, M. C. Majumder, K. P. Ramachandran, and Gulshan Taneja. "Reliability modeling and analysis of a two-unit parallel CC plant with different installed capacities." *Journal of Manufacturing Engineering* 5, no. 3 (2010): 197-204.
- [14] Mathew, A. G., S. M. Rizwan, M. C. Majumder, K. P. Ramachandran, and Gulshan Taneja. "Reliability analysis of identical two-unit parallel CC plant system operative with full installed capacity." *International Journal of Performability Engineering* 7, no. 2 (2011): 179-185.
- [15] Padmavathi, N., S. M. Rizwan, Anita Pal, and Gulshan Taneja. "Reliability analysis of an evaporator of a desalination plant with online repair and emergency shutdowns." *Aryabhatta Journal of Mathematics and Informatics* 4, no. 1 (2012): 1-12.
- [16] Padmavathi, N., S. M. Rizwan, Anita Pal, and Gulshan Taneja. "Comparative analysis of the two models of an evaporator of a desalination plant." In *Proc. of International Conference on Information and Mathematical Science*, Punjab, India, pp. 418-422. 2013.
- [17] Padmavathi, N., S. M. Rizwan, Anita Pal, and Gulshan Taneja. "Probabilistic analysis of an evaporator of a desalination plant with priority for repair over maintenance." *International Journal of Scientific and Statistical Computing* 4, no. 1 (2013): 1-9. https://doi.org/10.26634/jmat.2.1.2161
- [18] Padmavathi, N., S. M. Rizwan, Anita Pal, and Gulshan Taneja. "Probabilistic analysis of a desalination plant with major and minor failures and shutdown during winter season." *International Journal of Scientific and Statistical Computing* 5, no. 1 (2014): 15-23.
- [19] Padmavathi, N., S. M. Rizwan, Anita Pal, and Gulshan Taneja. "Probabilistic analysis of a seven unit desalination

- plant with minor/major failures and priority given to repair over maintenance." *Aryabhatta Journal of Mathematics and Informatics* 6, no. 1 (2014): 219-230.
- [20] Padmavathi, N., S. M. Rizwan, and A. Senguttuvan. "Comparative analysis between the reliability models portraying two operating conditions of a desalination plant." *International Journal of Core Engineering and Management* 1, no. 12 (2015): 1-10.
- [21] Rizwan, S. M., N. Padmavathi, and G. Taneja. "Performance analysis of a desalination plant as a single unit with mandatory shutdown during winter." *Arya Bhatta Journal of Mathematics and Informatics* 7, no. 1 (2015): 195-202.
- [22] Rizwan, S. M., N. Padmavathi, Anita Pal, and Gulshan Taneja. "Reliability analysis of a seven unit desalination plant with shutdown during winter season and repair/maintenance on FCFS basis." *International Journal of Performability Engineering* 9, no. 5 (2013): 523-528.
- [23] Rizwan, S. M., and Joseph V. Thanikal. "Reliability analysis of a waste water treatment plant with inspection." *i-manager's Journal on Mathematics* 3, no. 2 (2014): 21-26. https://doi.org/10.26634/jmat.3.2.3003
- [24] Rizwan, S. M., Joseph V. Thanikal, and Michel Torrijos. "A general model for reliability analysis of a domestic waste water treatment plant." *International Journal of Condition Monitoring and Diagnostic Engineering Management* 17, no. 3 (2014): 3-6.
- [25] Rizwan, S. M., Joseph V. Thanikal, N. Padmavathi, and Hathem Yazidi. "Reliability and availability analysis of an anaerobic batch reactor treating fruit and vegetable waste." *International Journal of Applied Engineering Research* 10, no. 24 (2015): 44075-44079.
- [26] Rizwan, S. M., and A. G. Mathew. "Performance analysis of port cranes." *International Journal of Core Engineering and Management* 2, no. 1 (2015): 133-140.
- [27] Al Rahbi, Yaqoob, S. M. Rizwan, B. M. Alkali, Andrew Cowel, and G. Taneja. "Reliability analysis of a subsystem in aluminium industry plant." In 2017 6th International Conference on Reliability, Infocom Technologies and Optimization (Trends and Future Directions)(ICRITO), pp. 199-203. IEEE, 2017. https://doi.org/10.1109/ICRITO.2017.8342424
- [28] Al Rahbi, Yaqoob, S. M. Rizwan, B. M. Alkali, Andrew Cowell, and G. Taneja. "Reliability analysis of rodding anode plant in aluminium industry." *International Journal of Applied Engineering Research* 12, no. 16 (2017): 5616-5623.
- [29] Al Rahbi, Yaqoob, S. M. Rizwan, B. M. Alkali, Andrew Cowell, and G. Taneja. "Maintenance analysis of a butt thimble removal system in aluminium plant." *International Journal of Mechanical Engineering and Technology* 9, no. 4 (2018): 695-703.
- [30] Al Rahbi, Yaqoob, S. M. Rizwan, B. M. Alkali, Andrew Cowell, and G. Taneja. "Reliability analysis of rodding anode plant in an aluminum industry with multiple repairmen." *Advances and Applications in Statistics* 53, no. 5 (2018): 569-597. https://doi.org/10.17654/AS053050569
- [31] Al Rahbi, Yaqoob, S. M. Rizwan, B. M. Alkali, Andrew Cowell, and G. Taneja. "Reliability analysis of a rodding anode plant in aluminum industry with multiple units failure and single repairman." *International Journal of System Assurance Engineering and Management* 10 (2019): 97-109. https://doi.org/10.1007/s13198-019-00771-3
- [32] Al Rahbi, Y., S. M. Rizwan, B. Alkali, A. Cowell, and G. Taneja. "Reliability analysis of multiple units with multiple repairmen of rodding anode plant in aluminum industry." *Advances and Applications in Statistics* 54, no. 1 (2019): 151-178. https://doi.org/10.17654/AS054010151
- [33] Al Rahbi, Yaqoob, and S. M. Rizwan. "A Comparative Analysis between the Models of a Single Component with Single Repairman & Multiple Repairmen of an Aluminium Industry." In 2020 International Conference on Computational Performance Evaluation (ComPE), pp. 132-135. IEEE, 2020. https://doi.org/10.1109/ComPE49325.2020.9200048
- [34] Taj, S. Z., S. M. Rizwan, B. M. Alkali, D. K. Harrison, and G. Taneja. "Reliability modelling and analysis of a single machine subsystem of a cable plant." In 2017 7th International Conference on Modeling, Simulation, and Applied Optimization (ICMSAO), pp. 1-4. IEEE, 2017. https://doi.org/10.1109/ICMSAO.2017.7934917
- [35] Taj, S. Z., S. M. Rizwan, B. M. Alkali, D. K. Harrison, and G. L. Taneja. "Reliability analysis of a single machine subsystem of a cable plant with six maintenance categories." *International Journal of Applied Engineering Research* 12, no. 8 (2017): 1752-1757.
- [36] Taj, S. Z., S. M. Rizwan, B. M. Alkali, D. K. Harrison, and Gulshan Taneja. "Reliability analysis of a 3-unit subsystem of a cable plant." *Advances and Applications in Statistics* 52, no. 6 (2018): 413-429. https://doi.org/10.17654/AS052060413
- [37] Taj, S. Z., S. M. Rizwan, B. M. Alkali, D. K. Harrison, and G. Taneja. "Performance and cost benefit analysis of a cable plant with storage of surplus produce." *International Journal of Mechanical Engineering and Technology* 9, no. 8 (2018): 814-826.
- [38] Taj, S. Z., S. M. Rizwan, B. M. Alkali, D. K. Harrison, and G. Taneja. "Profit analysis of a cable manufacturing plant portraying the winter operating strategy." *International Journal of Mechanical Engineering and Technology* 9, no. 11 (2018): 370-381.

- [39] Taj, S. Z., S. M. Rizwan, B. M. Alkali, D. K. Harrison, and G. Taneja. "Three reliability models of a building cable manufacturing plant: a comparative analysis." *International Journal of System Assurance Engineering and Management* 11 (2020): 239-246. https://doi.org/10.1007/s13198-020-01012-8
- [40] Taj, S. Z., and S. M. Rizwan. "Reliability modelling and analysis of complex industrial systems-a review." *i-manager's Journal on Mathematics* 8, no. 2 (2019): 43-60. https://doi.org/10.26634/jmat.8.2.16711
- [41] Rizwan, S. M., and S. Z. Taj. "Modeling and analysis of port PLCs." *Advances in Dynamical Systems and Applications* (ADSA) 16, no. 2 (2021): 423-440.
- [42] Kunalan, Kerishmaa Theavy, Cheng Yee Ng, and Nauman Riyaz Maldar. "A performance investigation of a multistaging hydrokinetic turbine for river flow." *Progress in Energy and Environment* 17 (2021): 17-31. https://doi.org/10.37934/progee.17.1.1731
- [43] Taj, S. Z., and S. M. Rizwan. "Estimation of reliability indices of a complex industrial system using best-fit distributions for repair/restoration times." *International Journal of Advanced Research in Engineering and Technology* 12, no. 2 (2021): 132-146.
- [44] Taj, S. Z., and S. M. Rizwan. "Reliability analysis of a 3-unit parallel system with single maintenance facility." *Advanced Mathematical Models & Applications* 7, no. 1 (2022): 93-103.
- [45] Taj, S. Z., S. M. Rizwan, B. M. Alkali, D. K. Harrison, and G. Taneja. "Probabilistic modeling and analysis of a cable plant subsystem with priority to repair over preventive maintenance." *i-manager's Journal on Mathematics (JMAT)* 6, no. 3 (2017): 12-21.
- [46] Taj, S. Z., S. M. Rizwan, B. M. Alkali, D. K. Harrison, and G. Taneja. "Performance analysis of a rod breakdown system." *International Journal of Engineering and Technology* 7, no. 3.4 (2018): 243-248. https://doi.org/10.14419/ijet.v7i3.4.16782
- [47] Misra, Krishna B. *Handbook of performability engineering*. Vol. 1256. London: Springer, 2008. https://doi.org/10.1007/978-1-84800-131-2